

Available online at [www.sciencedirect.com](http://www.sciencedirect.com)

ScienceDirect

Procedia CIRP 49 (2016) 199 – 202

[www.elsevier.com/locate/procedia](http://www.elsevier.com/locate/procedia)

The Second CIRP Conference on Biomanufacturing

## Design and Analysis of 3D Customized Models of a Human Mandible

Massimo Martorelli<sup>a,\*</sup>, Saverio Maietta<sup>a</sup>, Antonio Gloria<sup>b</sup>, Roberto De Santis<sup>b</sup>, Eujin Pei<sup>c</sup>,  
Antonio Lanzotti<sup>a</sup>

<sup>a</sup>Department of Industrial Engineering, Fraunhofer ILI IDEAS – University of Naples Federico II, P.le V. Tecchio 80, 80125 Naples, Italy<sup>b</sup>Institute of Polymers, Composites and Biomaterials - National Research Council of Italy, V.le J.F. Kennedy 54, 80125 Naples, Italy<sup>c</sup>Department of Design, College of Engineering Design and Physical Sciences - Brunel University London, Kingston Lane, Uxbridge, Middlesex UB8 3PH, UK\* Corresponding author. Tel.: +39 81 7682470; fax: +39 81 7682470. E-mail address: [massimo.martorelli@unina.it](mailto:massimo.martorelli@unina.it)

## Abstract

Polymer-based composites are ideal for applications where high strength-to-weight and stiffness-to-weight ratios are required. In the biomedical field, fiber-reinforced polymers have replaced metals, emerging as suitable alternative. Reverse engineering and additive manufacturing methods are required to achieve the design of customized devices with specific shape and size. At the same time, micro-mechanics and macro-mechanics play an important role in the development of highly functional composite materials.

The aim of this research is to develop customized 3D models of a human mandible using reverse engineering, additive manufacturing and composite material technology. Experiments were carried out by loading the models through the condyles and the results show the potential to reproduce the mechanical behavior of a human mandible. Taking into account the curves of the load-arch width decrease, the stiffness of the 3D composite model was  $14.1 \pm 1.9$  N/mm, which is close to the tested human mandible ( $17.5 \pm 1.8$  N/mm).

© 2015 The Authors. Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Peer-review under responsibility of the scientific committee of The Second CIRP Conference on Biomanufacturing

**Keywords:** Mandible; Reverse Engineering; Stereolithography; Fiber-reinforced composites; Experimental Testing

## 1. Introduction

Over the last decade, there have been great strides in the development of using emerging fabrication techniques and new materials for prosthetic and tissue engineering applications [1-36]. Acrylic mandibular models are often utilized for medical teaching, training and research. This work examines the process of developing and validating a synthetic human mandible that has implications for *in vitro* studies of dental implants and superstructures [25].

A key challenge in this area is the difficulty in finding cadaveric skeletal segments and the fact that the mechanical properties of the bone structure vary. The motivation of this work is to develop a realistic mandibular model that has close resemblance to the actual part in terms of geometry and its mechanical properties [37, 38].

The aim of this research is to enhance the design and development of a customized model of a human mandible using a combination of reverse engineering, additive manufacturing and composite materials. The properties of the produced model would be analyzed and compared to the current 3D polymeric and human mandibles.

Previous authors have developed different polymeric models of temporal bone by integrating reverse engineering with rapid prototyping techniques [1, 25, 39]. However, the design of the trabecular and cortical bones have not been properly modelled through synthetic models because they behave like homogeneous isotropic materials. In addition, the mechanical anisotropy of trabecular [40-44] and cortical bone [43-46] is also often neglected. Such anisotropic behavior can be observed in the trabecular bone of the condyle [47] and in the mandible body [48, 49] and the elastic modulus of those

parts vary along the different directional planes. Taking the mechanical properties of the human mandible in consideration, the mechanical anisotropy of cortical bone can be found in the mandible body [50] and in the ramus [39] as demonstrated through the elastic modulus [25].

Anisotropic edentulous mandible models made of a polymethylmethacrylate (PMMA) core and a glass fiber reinforced outer shell are often designed using reverse engineering methods and produced with composite materials [25, 37]. Medical grade samples use 3D customized models that consist of a PMMA-based bone cement as the core of the actual structure that simulates the trabecular bone, and an outer shell made of glass fiber reinforced epoxy composite to mimic the cortical bone. The glass fibers of the outer shell were oriented at angles of  $0^\circ$  and  $90^\circ$  with respect to the axis of the mandible corpus and at angles of  $\pm 45^\circ$  in the ramus to reproduce the cortical bone anisotropy. In our previous works [37, 38], the PMMA-based core was obtained through a multi-step procedure. A model of the core was first manufactured by inkjet printing and a silicone rubber mould was developed from the core prototype. The material was then poured into the customized mould.

In the current research the core was directly fabricated by additive manufacturing.

## 2. Materials and Methods

Three-dimensional (3D) composite edentulous mandibles were first produced using stereolithography (SLA) technique with composite materials. A 3D scan of a human mandible was performed using a Cyberware Mini Scanner and the data from the scanner was analyzed and repaired through the use of Rapid Form and Materialise Magics to ensure that the CAD geometries were water-tight and suitable for fabrication.

The inner core of the composite model consisted of a photo-curable acrylic resin with mechanical properties similar to that of trabecular bone. The outer shell of the mandible model consisted of a photo-curable glass fiber reinforced composite and this material was used for the core to simulate the compact bone anisotropy of the mandible arch.

To validate the polymeric and composite mandible models, experimental tests were designed and conducted by loading the composite models through the condyles up to a maximum load of 20 N. The testing conditions reproduce the loading configuration that are found in previous scientific work [51, 52]. An extensometer was used to record the local displacement in the symphysis region. Finally, the results were compared to those of a human mandible.

## 3. Results and Discussions

3D reconstructions of a human mandible were obtained from 3D scan data, using dedicated software such as Rapidform (Fig. 1a) and Magics (Fig. 1b).

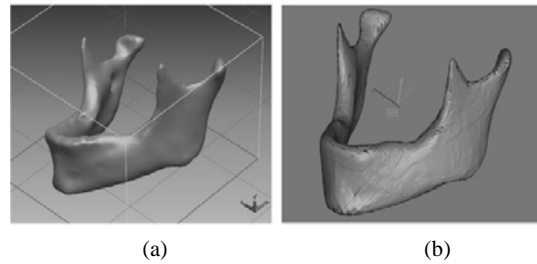


Fig. 1. 3D reconstructions of a human mandible obtained from 3D scan data, using dedicated software such as Rapidform (a) and Magics (b).

For the design of the mandible model, trabecular bone was replicated with an acrylic resin that has a Young's modulus of 2.0 GPa (Figure 2) and this value is close to that measured for trabecular bone (2.2 GPa) in the mandible symphysis and along the bucco-lingual direction [49]. The next step was to subject the human mandible on load-displacement tests as shown in Figure 3.



Fig. 2. Images of 3D customized polymeric (a) and composite models (b).

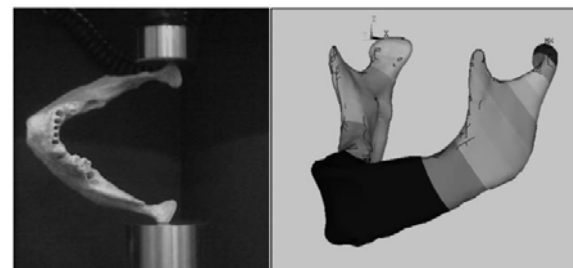


Fig. 3. Typical images of experimental and theoretical analyses performed on the human mandible.

Finally, the stiffness of both human and synthetic models were evaluated by examining the slope of the initial linear region of the load-displacement curves. Unlike the polymeric models, the composite model and the human mandible showed a load-arch width decrease curve which was linear up to the maximum load of 20 N (Fig. 4).

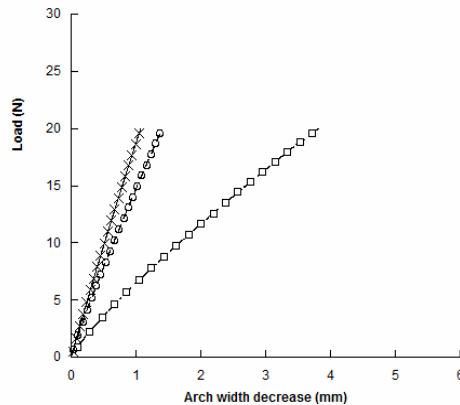


Fig. 4. Load-arch width decrease curves obtained from human mandible (x), polymeric (□) and composite (o) models.

The stiffness of the polymeric and composite models loaded through the condyles was  $5.1 \pm 0.5$  N/mm and  $14.1 \pm 1.9$  N/mm, respectively; while for the human mandible, a value of  $17.5 \pm 1.8$  N/mm was achieved. In line with Hobkirk and Schwab (1991), the load of pterygoid muscles at 16 N would equate to the reduction of 1 mm in terms of the distance between the condyles. As a consequence, the in-vitro stiffness of the mandible was 16 N/mm. The stiffness of the designed composite model is close to the values of a human mandible ( $17.5 \pm 1.8$  N/mm).

#### 4. Conclusions

The design and development of dental implants will improve the understanding of biomechanical features such as those for synthetic mandibles. Even though the geometry and size of these models can be easily obtained from 3D scanned data, the mechanical features of the part must be mechanically validated. Fiber-reinforced composite materials have played a crucial role in reproducing the anisotropy of the mandible cortical bone [44] and they have the potential to mimic the mechanical properties of natural hard tissues. By varying the fiber content and orientation as well as the composition of the matrix, we have demonstrated that we can tailor the mechanical properties of the materials to mimic the anisotropy of a human mandible [53]. Finally, this work has contributed to new knowledge by demonstrating the process of designing 3D mandibular models using reverse engineering, additive manufacturing and composite materials technology with the final product being validated through robust mechanical testing.

#### References

- [1] Gloria A, Ronca D, Russo T, D'Amora U, Chierchia M, De Santis R, Nicolais L, Ambrosio L. Technical features and criteria in designing fiber-reinforced composite materials: from the aerospace and aeronautical field to biomedical applications. *J Appl Biomater Biomech* 2011; 9: 151-163.
- [2] Lee J, Guarino V, Gloria A, Ambrosio L, Tae G, Kim YH, Jung Y, Kim SH, Kim SH. Regeneration of Achilles' tendon: the role of dynamic stimulation for enhanced cell proliferation and mechanical properties. *J Biomater Sci Polym Ed* 2010; 21: 1173-90.
- [3] Laino G, De Santis R, Gloria A, Russo T, Quintanilla DS, Laino A, Martina R, Nicolais L, Ambrosio L. Calorimetric and thermomechanical properties of titanium-based orthodontic wires: DSC-DMA relationship to predict the elastic modulus. *J Biomater Appl* 2012; 26: 829-44.
- [4] Gloria A, Borzacchiello A, Causa F, Ambrosio L. Rheological Characterization of Hyaluronic Acid Derivatives as Injectable Materials Toward Nucleus Pulposus Regeneration. *J Biomater Appl* 2012; 26: 745-759.
- [5] Esposito AR, Moda M, de Melo Cattani SM, de Santana GM, Abreu Barbieri J, Moron Munhoz M, Pereira Cardoso T, Peris Barbo ML, Russo T, D'Amora U, Gloria A, Ambrosio L, de Rezende Duek EA. PLDLA/PCL-T Scaffold for Meniscus Tissue Engineering. *BioRes Open Access* 2013; 2: 138-147.
- [6] Giordano C, Albani D, Gloria A, Tunesi M, Batelli S, Russo T, Forloni G, Ambrosio L, Cigada A. Multidisciplinary perspectives for Alzheimer's and Parkinson's diseases: hydrogels for protein delivery and cell-based drug delivery as therapeutic strategies. *Int J Artif Organs* 2009; 32: 836-850.
- [7] Giordano C, Albani D, Gloria A, Tunesi M, Rodilossi S, Russo T, Forloni G, Ambrosio L, Cigada A. Nanocomposites for neurodegenerative diseases: hydrogel-nanoparticle combinations for a challenging drug delivery. *Int J Artif Organs* 2011; 34: 1115-27.
- [8] Guarino V, Gloria A, Raucci MG, Ambrosio L. Hydrogel-Based Platforms for the Regeneration of Osteochondral Tissue and Intervertebral Disc. *Polymers* 2012; 4: 1590-1612.
- [9] Russo T, Gloria A, D'Antò V, D'Amora U, Ametrano G, Bollino F, De Santis R, Ausanio G, Catauro M, Rengo S, Ambrosio L. Poly( $\epsilon$ -caprolactone) reinforced with sol-gel synthesized organic-inorganic hybrid fillers as composite substrates for tissue engineering. *J Appl Biomater Biomech* 2010; 8: 146-152.
- [10] Puppi D, Mota C, Gazzarri M, Dinucci D, Gloria A, Myzabekova M, Ambrosio L, Chiellini F. Additive manufacturing of wet-spun polymeric scaffolds for bone tissue engineering. *Biomedical Microdevices* 2012; 14: 1115-1127.
- [11] Antunes JC, Pereira CL, Molinos M, Ferreira da Silva F, Dessì M, Gloria A, Ambrosio L, Gonçalves RM, Barbosa MA. Layer-by-Layer Self-Assembly of Chitosan and Poly( $\gamma$ -glutamic acid) into Polyelectrolyte Complexes. *Biomacromolecules* 2011; 12: 4183-4195.
- [12] Gloria A, Causa F, Russo T, et al. Three-Dimensional Poly( $\epsilon$ -caprolactone) Bioactive Scaffolds with Controlled Structural and Surface Properties. *Biomacromolecules* 2012; 13: 3510-21.
- [13] Domingos M, Chiellini F, Gloria A, Ambrosio L, Bartolo P, Chiellini E. Effect of process parameters on the morphological and mechanical properties of 3D Bioextruded poly( $\epsilon$ -caprolactone) scaffolds. *Rapid Prototyp J* 2012; 18: 56-67.
- [14] Domingos M, Intranuovo F, Gloria A, Gristina R, Ambrosio L, Bártolo PJ, Favia P. Improved osteoblast cell affinity on plasma-modified 3D-extruded PCL scaffolds. *Acta Biomaterialia* 2013; 9: 5997-6005.
- [15] Reitmaier S, Wolfram U, Ignatius A, Wilke HJ, Gloria A, Martín-Martínez JM, Silva-Correia J, Oliveira JM, Reis RL, Schmidt H. Hydrogels for nucleus replacement – facing the biomechanical challenge. *J Mech Behav Biomed Mater* 2012; 14: 67-77.
- [16] Silva-Correia J, Gloria A, Oliveira MB, Mano JF, Oliveira JM, Ambrosio L, Reis RL. Rheological and mechanical properties of acellular and cell-laden methacrylated gellan gum hydrogels. *J Biomed Mater Res A* 2013; 101: 3438-46.
- [17] Russo T, D'Amora U, Gloria A, Tunesi M, Sandri M, Rodilossi S, Albani D, Forloni G, Giordano C, Cigada A, Tampieri A, De Santis R, Ambrosio L. Systematic Analysis of Injectable Materials and 3D Rapid Prototyped Magnetic Scaffolds: From CNS Applications to Soft and Hard Tissue Repair/Regeneration. *Procedia Eng* 2013; 59: 233-239.
- [18] De Santis R, Gloria A, Russo T, D'Amora U, Zeppetelli S, Dionigi C, Sytcheva A, Herrmannsdörfer T, Dediu V, Ambrosio L. A basic approach toward the development of nanocomposite magnetic scaffolds for advanced bone tissue engineering. *J Appl Pol Sci* 2011; 122: 3599-360.
- [19] Banobre-Lopez M, Pineiro-Redondo Y, De Santis R, Gloria A, Ambrosio L, Tampieri A, Dediu V, Rivas J. Poly(caprolactone) based

- magnetic scaffolds for bone tissue engineering. *J Appl Phys* 2011; 109: 07B313-1 - 07B313-3.
- [20] Gloria A, Russo T, D'Amora U, Zeppetelli S, D'Alessandro T, Sandri M, Bañobre-López M, Piñeiro-Redondo Y, Uhlarz M, Tampieri A, Rivas J, Herrmannsdörfer T, Dediu VA, Ambrosio L, De Santis R. Magnetic poly( $\epsilon$ -caprolactone)/iron-doped hydroxyapatite nanocomposite substrates for advanced bone tissue engineering. *J R Soc Interface* 2013; 10: 20120833-1 – 20120833-11
- [21] De Santis R, Gloria A, Russo T, D'Amora U, D'Antò V, F. Bollino, M. Catauro, F. Mollica, S. Rengo, L. Ambrosio. Advanced composites for hard-tissue engineering based on PCL/organic-inorganic hybrid fillers: From the design of 2D substrates to 3D rapid prototyped scaffolds. *Polymer Composites* 2013; 34: 1413-1417.
- [22] Domingos M, Intranuovo F, Russo T, De Santis R, Gloria A, Ambrosio L, Ciurana J, Bartolo P. The first systematic analysis of 3D rapid prototyped poly( $\epsilon$ -caprolactone) scaffolds manufactured through BioCell printing: the effect of pore size and geometry on compressive mechanical behaviour and in vitro hMSC viability. *Biofabrication* 2013; 5: 045004-1 – 045004-13.
- [23] De Santis R, Russo A, Gloria A, D'Amora U, Russo T, Panseri S, Sandri M, Tampieri A, Maracci M, Dediu VA, Wilde CJ, Ambrosio L. Towards the Design of 3D Fiber-Deposited Poly( $\epsilon$ -caprolactone)/Iron-Doped Hydroxyapatite Nanocomposite Magnetic Scaffolds for Bone Regeneration. *Journal of Biomedical Nanotechnology* 2015; 11: 1236–1246.
- [24] Tsaryk R, Gloria A, Russo T, Anspach L, De Santis R, Ghanaati S, Unger RE, Ambrosio L, Kirkpatrick CJ. Collagen-low molecular weight hyaluronic acid semi-interpenetrating network loaded with gelatin microspheres for cell and growth factor delivery for nucleus pulposus regeneration. *Acta Biomaterialia* 2015; 20: 10–21.
- [25] De Santis R, Sarracino F, Mollica F, Netti PA, Ambrosio L, Nicolais L. Continuous fibre reinforced polymers as connective tissue replacement. *Compos Sci Technol* 2004; 64: 861-71.
- [26] Lanzotti A, Martorelli M, Staiano G. Understanding Process Parameter Effects of RepRap Open-Source Three-Dimensional Printers Through a Design of Experiments Approach. *J Manuf Sci Eng* 2015; 137(1): 7 pages. Paper No: MANU-14-1207; doi: 10.1115/1.4029045.
- [27] Martorelli M, Ausiello P, Morrone R. A new method to assess the accuracy of a Cone Beam Computed Tomography scanner by using a non-contact reverse engineering technique. *Journal of dentistry* 2014; 42: 460-465.
- [28] Martorelli M. A new approach in CT artifact removal: three cases study in maxillofacial surgery. *International Journal on Interactive Design and Manufacturing* 2013; 7: 115-124.
- [29] Giordano M, Ausiello P, Martorelli M. Accuracy evaluation of surgical guides in implant dentistry by non-contact reverse engineering techniques. *Dental Materials* 2012; 28: e178-e185.
- [30] Martorelli M., Gerbino S., Giudice M., Ausiello P., A comparison between customized clear and removable orthodontic appliances manufactured using RP and CNC techniques, *Dental Materials*, 2013, 29(2), pp. 1-10, ISSN 0109-5641, Publisher Elsevier.
- [31] Martorelli M, Ausiello P. A novel approach for a complete 3D tooth reconstruction using only 3D crown data, *International Journal on Interactive Design and Manufacturing*, 2013, 7(2), pp. 125–133, ISSN 1955-2513, Publisher Springer.
- [32] Ausiello P., Franciosa P., Martorelli M., Watts D.C., Effects of Thread Features in Osseo-Integrated Titanium Implants using a Statistics-based Finite Element Method, *Dental Materials*, 2012, 28(8), pp. 919-927, ISSN 0109-5641, Publisher Elsevier.
- [33] Giordano M., Ausiello P., Martorelli M., Sorrentino R., Reliability of computer designed surgical guides in six implant rehabilitations with two years follow-up, *Dental Materials*, 2012, 28(9), pp. 168-177, Publisher Elsevier.
- [34] Franciosa P, Martorelli M. Stress-based performance comparison of dental implants by finite element analysis. *International Journal on Interactive Design and Manufacturing* 2012, 6(2), pp. 123–129, ISSN 1955-2513, Publisher Springer.
- [35] Ausiello P., Franciosa P., Martorelli M., Watts D.C., Numerical fatigue 3D-FE modelling of indirect composite-restored posterior teeth, *Dental Materials*, 2011, 27 (5), pp. 423-430, ISSN 0109-5641, Publisher Elsevier.
- [36] Ausiello P., Franciosa P., Martorelli M., Watts D.C., Mechanical behavior of post-restored upper canine teeth: A 3D FE analysis, *Dental Materials*, 2011, 27(12), pp. 1285-1294, ISSN 0109-5641, Publisher Elsevier.
- [37] De Santis R, Mollica F, Esposito R, Ambrosio L, Nicolais L. An experimental and theoretical composite model of the human mandible. *J. Mater Sci: Mater Med* 2005; 16: 1191–1197.
- [38] De Santis R, Gloria A, Russo T, D'Amora U, Varriale A, Veltri M, Balleri P, Mollica F, Riccitiello F, Ambrosio L. Reverse engineering of mandible and prosthetic framework: Effect of titanium implants in conjunction with titanium milled full arch bridge prostheses on the biomechanics of the mandible. *J Biomech* 2014; 47:3825-9.
- [39] Hara T, Takizawa M, Sato T, Ide Y. Mechanical properties of buccal compact bone of the mandibular ramus in human adults and children: relationship of the elastic modulus to the direction of the osteon and the porosity ratio. *Bull Tokyo Dent Coll* 1998; 39: 47-55.
- [40] Zysset, PK, Guo, XE, Hoffer, CE, Moore, KE and Goldstein, SA. Elastic modulus of human cortical and trabecular tissue lamella. *J Biomech* 1999; 32: 1005-12.
- [41] Rho JY, Ashman RB, Turner CH. Young's modulus of trabecular and cortical bone material: Ultrasonic and microtensile measurements. *J Biomech* 1993; 26: 111-9.
- [42] Keaveny TM, Wachtel EF, Ford CM, Hayes WC. Differences between the tensile and compressive strengths of bovine tibial trabecular bone depend on modulus. *J Biomech* 1994; 9: 1137-46.
- [43] De Santis R, Ambrosio L, Mollica F, Netti P, Nicolais L. Mechanical properties of human mineralized connective tissues. Modeling of Biological Materials. In: Mollica F, Preziosi L, Rajagopal KR, editors. *Modeling of Biological Materials*. Boston: Birkhäuser; 2007. p. 211-261.
- [44] De Santis R, Ambrosio L, Nicolais L. Mechanical properties of tooth structures. In: Barbucci R, editors. *Integrated Biomaterials Science*. Springer US: Kluwer Academic Publishers 2002. p. 589-599.
- [45] Reilly DT, Burstein AH, Krinkel VH. The elastic modulus of bone. *J Biomech* 1974; 7: 271-5.
- [46] Liu D, Weiner S, Wagner HD. Anisotropic mechanical properties of lamellar bone using miniature cantilever bending specimens. *J Biomech* 1999; 32: 647-54.
- [47] Giesen EBW, Ding M, Dalstra M, van Eijden TMGJ. Mechanical properties of cancellous bone in the human mandibular condyle are anisotropic. *J Biomech* 2001; 34: 799-803.
- [48] Misch CE, Qu Z, Bidez MW. Mechanical properties of trabecular bone in the human mandible: implications for dental implant treatment planning and surgical placement. *J Oral Maxillofac Surg* 1999; 57: 700-6.
- [49] O'Mahony AM, Williams JL, Katz JO, Spencer P. Anisotropic elastic properties of cancellous bone from a human edentulous mandible. *Clin Oral Implants Res* 2000; 11: 415-21.
- [50] Tamatsu Y, Kaimoto K, Arai M, Ide Y. Properties of the elastic modulus from buccal compact bone of human mandible. *Bull Tokyo Dent Coll* 1996; 37: 93-101.
- [51] Hobkirk JA, Schwab J. Mandibular deformation in subjects with osseointegrated implants. *Int J Oral Maxillofac Implants* 1991; 6: 319-28.
- [52] Zarone F, Apicella A, Nicolais L, Aversa R, Sorrentino R. Mandibular flexure and stress build-up in mandibular full-arch prostheses supported by osseointegrated implants. *Clin Oral Implant Res* 2003; 14: 103–114.
- [53] Schwartz-Dabney CL, Dechow PC. Variations in cortical material properties throughout the human dentate mandible. *Am J Phys Anthropol* 2003; 120: 252–277.